



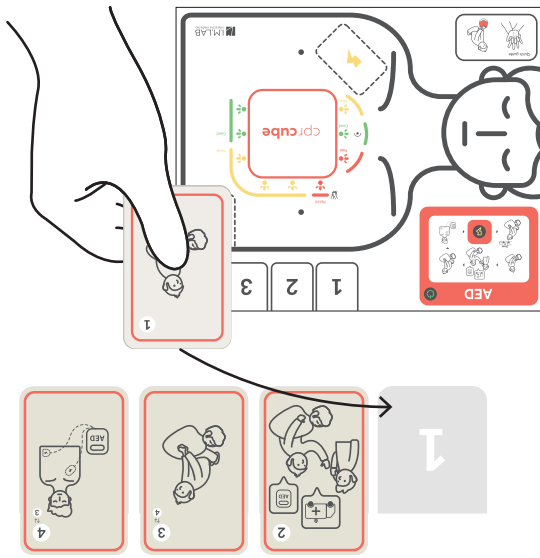

MATCHING SCENARIO CARDS

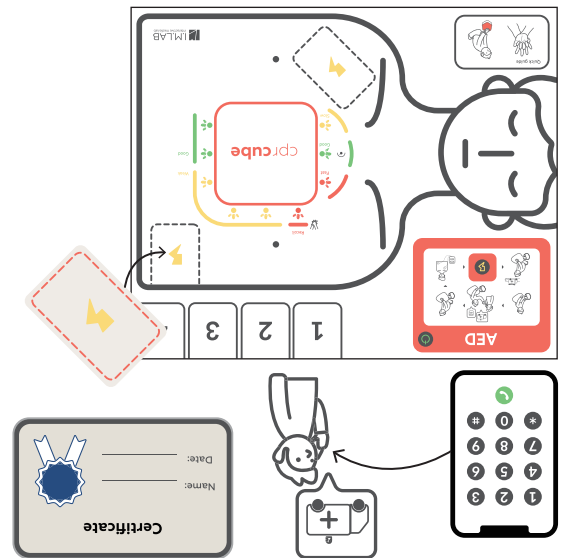


ROLE PLAYING

WARRANTY

1. Manufacturer offers a LIMITED WARRANTY against any defects in workmanship or materials under normal use for one (1) year from the date of purchase. Any component of the cprCUBE which proves defective within the warranty period will be repaired, free of charge. The customer is responsible for shipping and handling fees to the place which manufacturer designates.
2. Customer must provide proof of the date of purchase, place of purchase and the purchase price in order to obtain service under this limited warranty. No agent, representative, dealer of Manufacturer has the authority to alter the obligations or limitations of this limited warranty.
3. CUSTOMER'S SOLE AND EXCLUSIVE REMEDY AGAINST MANUFACTURE SHALL BE FOR THE REPAIR OR REPLACEMENT OF DEFECTIVE GOODS AS PROVIDED HEREIN. Repair of any component of any cprCUBE does not extend this limited warranty or begin a new limited warranty period.
4. Manufacturer reserves the right to refuse warranty service or replacement when product failure is due to abrasion, abnormal use, misuse, mishandling, misapplication, accident, neglect, improper installation, modification, use of unauthorized parts or attachments, adjustments or repair performed by anyone other than manufacturer or its authorized agent, or any causes other than defective workmanship or material. This limited warranty does not cover failure or damage resulting from unsuitable operating environments or storing environments or natural disasters or acts of God. MANUFACTURE SHALL NOT BE LIABLE FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES ARISING OUT OF THE USE OF THE cprCUBE OR THE BREACH OF THIS OR ANY OTHER EXPRESSED OR IMPLIED WARRANTY.

1. 제조자는 구매일로부터 일 (1) 년 동안 정상적인 사용 상태에서의 제작상의 또는 부품의 결함에 대해 제한적 보증을 제공합니다. 구매일로부터 12개월 이내에 결함이 있는 것으로 판명 된 제품은 무료로 수리됩니다. 구매자는 업체가 지정한 장소로 운송 및 취급 수수료를 지불해야 합니다.
2. 구매자는 제한적 보증에 명시된 서비스를 받으려면 구입 날짜, 구매 장소 및 구매 가격을 증명해야 합니다. 제조사의 에이전트 또는 판매원은 이 제한적 보증의 의무 또는 제약을 변경할 수 있는 권한이 없습니다.
3. 제조자에 대한 제품구매자의 유일한 배타적 보증은 여기에 명시된 결함 제품의 수리를 위한 것입니다. cprCUBE 의 수리로 인하여 기존 보증기간의 연장 또는 새로운 보증 기간의 시작이 적용되지 않습니다.
4. 제조자는 잘못된 사용, 취급부주의, 사고, 부적절한 설치, 잘못된 적용에 의한 오용, 개조, 승인되지 않은 부품 또는 첨부물의 사용, 또는 승인 된 사람 이외의 사람이 수행 한 수리 또는 개조로 인한 제품 고장 및 제조결함 이외의 원인에 대하여는 보증 서비스를 제공하지 않습니다. 또한, 제한적 보증은 마모, 비정상적인 사용, 부주의로 인한 손상, 무단 개조, 제품의 사용이 부적합한 환경에서의 사용이나 보관으로 인해 발생한 손상, 자연재해 및 천재지변에 의한 손상에 관해서는 보상하지 않습니다. 제조자는 cprCUBE의 미사용에 의한 우발적 혹은 필연적 손해 또는 기타 다른 명시적 또는 묵시적 보증의 위반으로 인한 경우 발생하는 손해에 대해 책임지지 않습니다.





cprcube™

2ND GENERATION

USER GUIDE

COMPONENTS

- ① User Guide
- ② Scenario cards
- ③ cprcube Board
- ④ cprcube

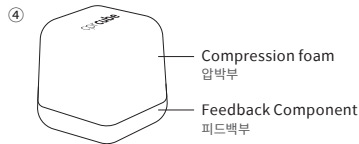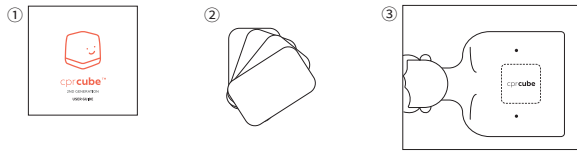

* Batteries are not included (4 AA batteries needed)
Alkaline batteries are recommended for this product.


AA 배터리는 포함되어 있지 않습니다. (4개 필요)
본 제품에는 알카라인 건전지를 사용하시는 것을 권장합니다.

Online guide for
cprcube



HOW TO USE

① Insert Batteries



② Turn On/Off


- Push once to turn on
한 번 눌러 전원을 켭니다.
- Push for 2 seconds to turn off
2초 간 눌러 전원을 끕니다.

When the device turn On/Off,
LEDs light and melody sounds
전원 On/Off 시 LED와 알람음이 작동합니다.

The device turns off with no action
more than 10 minutes
10분 이상 동작하지 않으면 자동으로 꺼집니다.

③ Place on the Board

Unfold the board and place cprCUBE
main body matching the logo orientation
접힌 보드를 잘 펴준 뒤, 로고 방향에 맞춰 큐브를
올려 놓습니다



Guide Mode

Compress cprCUBE main body for more
than 3 seconds to activate guide mode
큐브를 3초 간 꼭 누르고 있으면 가이드 모드로
전환됩니다. (가이드 모드가 시작되면 메트로놈
음이 반복됩니다.)



FEEDBACK

LED Feedback

Compression
Rate feedback
속도 피드백



- Fast 빠른
(≥120CPM)
- Good 좋음
(100~120CPM)
- Slow 느림
(≤120CPM)

Recoil feedback
이완 피드백



- Recoil needed
이완 부족
(≤1cm)

Compression
Depth feedback
깊이 피드백



- Good 좋음
(≥5cm)
- Weak 약함
(<5cm)

Sound Feedback

Correct compression
정확한 압박



Incorrect compression
잘못된 압박



10, 20, 30 combos
10, 20, 30 콤보



PRODUCT INFORMATION

Product name cprcube
Model number CC2G
MFR/Country I.M.LAB Inc. / Made in China
Certifier Identification code KC ID: R-R-IML-CC2G
Class B Device(Б급 기기)

Product Specification

cprcube Board		cprcube	
Dimension	100×110×0.5 (mm) (Folded) 400×330 (mm) (Unfolded)	Dimension	100×100×110(mm)
Weight	17.5g	Weight	245g
		Power supply	6.0V (4 AA alkaline batteries)

FCC Part 15 B

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures: - Reorient or relocate the receiving antenna. / - Increase the separation between the equipment and receiver. / - Connect the equipment into an outlet on a circuit different from that to which the receiver is connected. / - Consult the dealer or an experienced radio/TV technician for help.

FCC Part 15.19

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

FCC Part 15.21

Any changes or modifications (including the antennas) to this device that are not expressly approved by the manufacturer may void the user's authority to operate the equipment.

⚠ CAUTION

- Keep the used batteries out of reach of children and dispose separately.
- If you do not use the device for a long period of time remove and store the batteries.
- Do not use a new battery and an old battery together.



E-mail. contact@imlabworld.com
Tel. +82-70-5056-3900 Fax. +82-505-170-3900
7F, 165, Yeoksam-ro, Gangnam, Seoul, South Korea
서울특별시 강남구 역삼로 165, 7층 아이엠랩